

## **INSPECTION REPORT**

### **Sedecal X Plus LP +**

**RENOVA MEDİKAL  
MÜHENDİSLİK TİC. A.Ş.**

Oruçreis Mh. Giyimkent Cd.  
Giyimkent Sitesi No: 86-88  
Esenler / İstanbul

T. 0 850 226 26 22  
F. 0 212 438 48 96

[renovamedikal.com.tr](http://renovamedikal.com.tr)

**GENERAL INFORMATION**

Brand	SEDECAL
Model	X PLUS LP +
Y.O.M	2011

**TUBE INFORMATION**

Tube YOM	
Tube Type	

**WORKSTATION INFORMATION**

SW Version	
SW Options	

**COLIMATOR**

Type	
Model No	

**DETECTOR**

Type	
Model No	

**RENOVA MEDİKAL  
MÜHENDİSLİK TİC. A.Ş.**

Oruçreis Mh. Giyimkent Cd.  
Giyimkent Sitesi No: 86-88  
Esenler / İstanbul

T. 0 850 226 26 22  
F. 0 212 438 48 96

[renovamedikal.com.tr](http://renovamedikal.com.tr)

## CABINET

---

Type	
Model No	

## COSMETIC CONDITION

---

## OTHER NOTES

---

## QA

---

Inspection done by & Date:


**RENOVA MEDİKAL  
MÜHENDİSLİK TİC. A.Ş.**

Oruçreis Mh. Giyimkent Cd.  
Giyimkent Sitesi No: 86-88  
Esenler / İstanbul

T. 0 850 226 26 22  
F. 0 212 438 48 96

[renovamedikal.com.tr](http://renovamedikal.com.tr)

**SYSTEM PHOTOS**

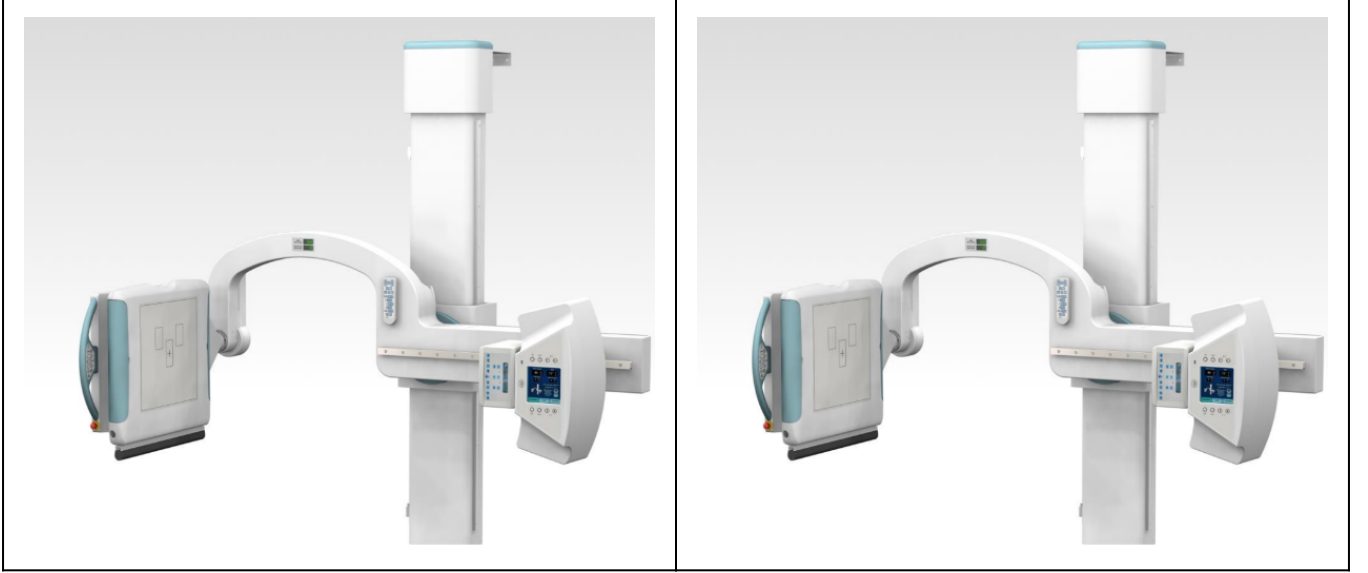

**RENOVA MEDİKAL  
MÜHENDİSLİK TİC. A.Ş.**

Oruçreis Mh. Giyimkent Cd.  
Giyimkent Sitesi No: 86-88  
Esenler / İstanbul

T. 0 850 226 26 22  
F. 0 212 438 48 96

[renovamedikal.com.tr](http://renovamedikal.com.tr)